

Quantitative Analysis of Water Content and Distribution in Plants using Terahertz Imaging

A.V. Shchepetilnikov^{a,b,*}, A.M. Zarezin^{a,b,c}, V.M. Muravev^{a,b}, P.A. Gusikhin^{a,b}, I.V. Kukushkin^{a,b}

^aInstitute of Solid State Physics, RAS, Chernogolovka, 142432 Russia

^bTeraSense Group, Inc., San Jose, CA, 95110 USA

^cMoscow Institute of Physics and Technology, Dolgoprudny, 141700 Russia

Abstract. Quantitative analysis of the temporal evolution and spatial distribution of water content in grass and clover leaves has been carried out *in vivo*, with the aid of the terahertz imaging system comprised of an IMPATT-diode source, a condenser lens, and an imaging camera. The leaf samples were exposed to 100 GHz radiation to measure the transmitted power. Progressive variation in the level of the transmitted signal has been detected when the plants were subject to the condition of insufficient water supply, whereas after watering the plants, the transmission was restored to its initial value. The presented experimental results demonstrate that TeraSense imaging instrumentation can be used effectively to monitor the hydration state of plants in their natural environment.

Keywords: terahertz imaging, plants hydration status.

*A.V. Shchepetilnikov, shchepetilnikov@issp.ac.ru

1 Introduction

Terahertz (THz) radiation corresponds to electromagnetic spectrum between 0.1 and 1 THz (1 – 100 meV). Many molecules exhibit strong absorption in the THz frequency band due to their rotational and vibrational transitions. This molecular property opens up promising opportunities for various prospective applications of THz imaging in bioscience.¹ Possible practical areas of interest may include non-invasive detection of cells and tissues,^{2,3} non-destructive crop and seed separation,^{4,5} and monitoring water content in living cells of humans and plants.⁶ To make the transition from a laboratory-scale terahertz imaging technique to an industrial-grade technology, a slow and cumbersome, single-pixel, raster-scanning systems need to be replaced with fast, cutting-edge multipixel cameras. Such advanced imaging systems become particularly critical in high-throughput conveyor applications. In this manuscript, we present a detailed study of the evolution of plant hydration accomplished employing a semiconductor multipixel THz camera. The primary

objective of our investigation has been to make terahertz technology more practical and versatile for a broad range of bioscience applications.

The level of water content in plants is one of the key parameters to monitor at nearly every stage of their cultivation process. On the one hand, inadequate hydration can lead to a significant reduction in the quality and quantity of the yield, whereas prolonged or severe water stress may even result in the death of the crop. On the other hand, over-irrigation is not only economically inefficient due to excessive use of water resources, but can also harm the plants by impairing soil aeration and thereby increasing their vulnerability to certain pests and diseases. Therefore, it is vital to determine the acceptable dehydration level of a plant not to be destructive to it or to undermine its normal growth and productiveness.

Traditionally, the hydration state of a plant as a whole is monitored by measuring the water content of its leaves.⁷ This quantity can be extracted from the analysis of their transmission and reflection data obtained in the terahertz (THz) frequency range. Unlike most dehydrated biological tissues that are transparent to THz radiation, water is extremely adsorbent in this frequency range.^{8,9} Thus, even relatively small variations of water amount contained in the leaves result in drastic changes in their THz optical properties.^{10–15} Such fluctuations can be sensed easily by means of contemporary THz imaging techniques. For instance, present-day THz technologies are elaborate enough to perform industrial-scale, non-destructive product quality control^{16–20} and even security screening.^{21,22}

In non-destructive testing (NDT) performed at THz frequencies, there are two conventional approaches: the time-domain spectroscopy,^{23,24} and the continuous wave (*cw*) schemes.^{25,26} The former is based on irradiating a sample with short electromagnetic pulses, and analyzing the resultant transmitted or reflected signal. Although this technique provides detailed information about

the sample absorption or reflection spectra over the entire THz frequency band, a typical setup is highly complex and costly, with a rather slow measurement rate. The latter method, on the other hand, is considerably simpler, faster, and more cost-effective, as it allows for implementation of fairly compact and portable, commercially available solutions. Recently, there have been reported a number of *cw* imagers operating at a single radiation frequency,^{26–32} including several systems developed by our group at TeraSense.^{33–36}

In this paper, we adapt the aforementioned TeraSense instrumentation to the study of water content in plant leaves. In the proposed arrangement, the incident CW radiation generated with a standard IMPATT-diode source at 100 GHz propagates through a leaf sample and is then detected by an imaging camera,^{33,34} which permits the analysis of the transmission pattern of the sample and, hence, of the water distribution inside the leaves. **The chosen frequency matches one of the atmospheric microwave windows³⁷ ensuring the low loss of the microwave power propagating through the air volume.** The suggested measurement approach has several key advantages over conventional destructive techniques like thermogravimetric methods. It fully preserves the integrity of the test sample, as THz radiation at moderate power levels has a negligible effect on the plants. Second, it enables remote monitoring of leaves' water content in real-time so that the dynamics of plant hydration could be studied under various conditions. Furthermore, THz imaging technology facilitates the analysis of the spatial distribution of water within the leaves.

2 System description

In our experiments, we used the system configuration depicted schematically in Fig. 1(A). In this arrangement, the radiation produced by the IMPATT-diode source is emitted from the horn antenna attached directly to the output waveguide flange of the generator. To achieve a nearly non-divergent

radiation beam, we used an aspherical PTFE beam-collimating lens with a focal distance of 50 mm. The beam spot was made sufficiently large to cover the full pixel-array area of the imaging camera. Photographs of both the source and the camera are shown in Fig. 1(B) and (C), respectively. The source operated at a fixed output power level of approximately 80 mW, and a single frequency of 96 GHz with 1 MHz linewidth, as determined by the measurements taken with the Agilent E4407B spectrum analyzer along with the Agilent 11970W harmonic mixer, and the VDI Erickson PM5 power meter.

The heart of the system is its real-time imaging camera (Fig. 1 (C)), which relies on a new method of plasmonic detection^{38,39} that makes possible ultra-fast sensing of THz radiation at room temperature. The camera has an array of 32×32 pixels with $1.5 \times 1.5 \text{ mm}^2$ pitch, and a single-pixel size of $1.3 \times 1.3 \text{ mm}^2$. At 96–98 GHz, the effective responsivity of each pixel is $50 \pm 10 \text{ kV/W}$, and the corresponding noise equivalent power is $1 \text{ nW/Hz}^{1/2}$. The image acquisition rate of the camera was set to 24 frames per second. The overall imaging system is controlled by a PC through a specially designed software.

To estimate the dynamics and spatial distribution of the water content inside the leaves, we acquired the transmission pattern of several leaf samples with each sample placed directly on the imaging camera. The distance between the leaf surface and the detector array was equal to 4 mm. The power of the incident beam was normalized by a reference image recorded when no object was present on the camera. Figures 1 (D) and (E) show a photo of a tree leaf and its sub-THz image reconstructed from several 32×32 pixels images. The colors indicate the transmission coefficient values. Notably, the inner structure of the leaf is clearly resolved in the obtained image. In our investigation, we focused primarily on two plant species that are important in agriculture, namely the clover and grass. We measured the transmission patterns of different leaves over several days,

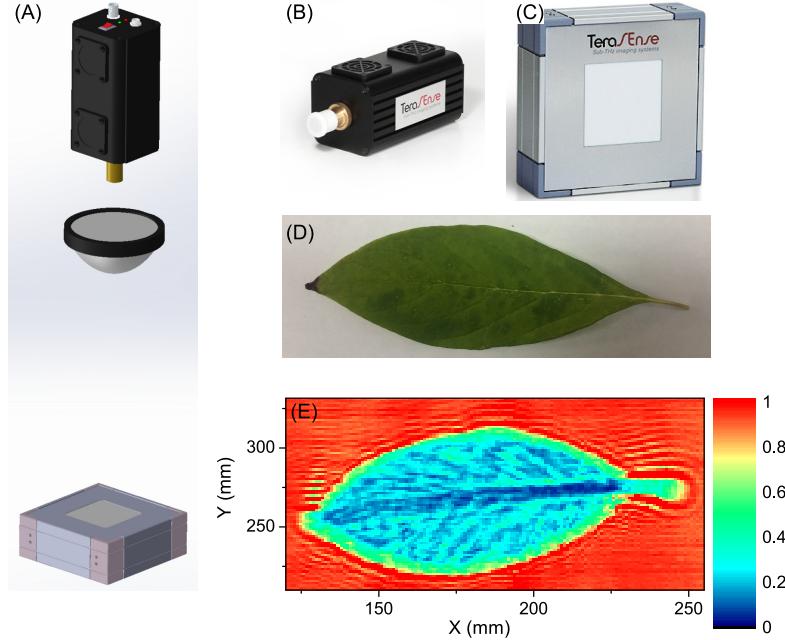


Fig 1 (A) Schematic illustration of the experimental setup. The radiation beam produced by the IMPATT-diode source is collimated by a PTFE lens with a focal distance of 50 mm. The power distribution within the beam is probed with the imaging camera. (B) and (C) Photos of the camera and the IMPATT source. (D) and (E) A regular, visible light photo and a sub-THz image of a tree leaf. Image colors indicate the transmission coefficient values.

while the plants growing in the pots were subject to water-restricted conditions.

3 Measurement results

Figure 2 displays transmission data for three clover leaves tested during a 6-day period without watering. The blue open symbols represent dependence of transmission averaged over the number of camera pixels. In order to average transmission coefficient three areas of a leaf were taken. In particular, rectangular sections of 5×6 pixels in size, chosen approximately at the center of each leaf. Then transmission values of all those pixels was averaged giving solid line on the Figure 2. Over the entire test period, the blue curve illustrates a marked change in the transmission that almost tripled in value after 6 days without watering the plant, which reflects a substantial decrease in the leaf water content. Notably, there is a plateau with approximately constant transmission value during the first 3 days and the subsequent rise. Figures 2 (a,b,c) include sub-THz images

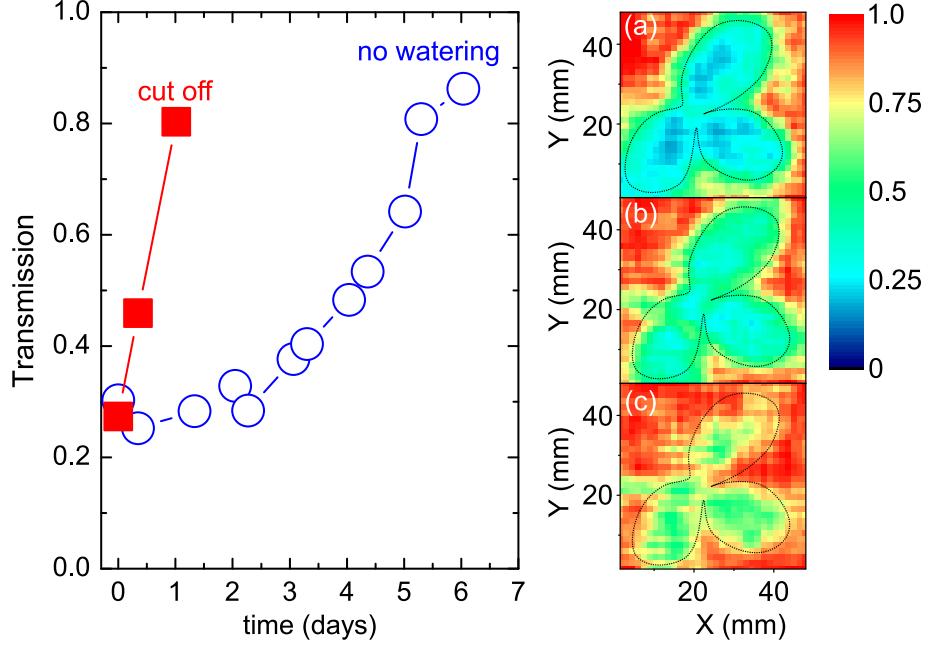


Fig 2 Changes in the transmission of a sub-THz signal through the leaf of clover. The blue curve with empty circles denotes the time evolution of the transmission through the leaf samples of a plant subject to water restricted conditions. The respective sub-THz images of the clover leaves, (a), (b), (c) illustrate different hydration levels measured on the first, third, and fifth days of the experiment. Image colors correspond to the value of the transmittance. The red curve with solid points represents an analogous dependence for the leaf cut-off from the same plant.

denoting the transmission patterns of the clover leaves recorded on the first, third and fifth days of the experiment. The images help to visualize the progressive reduction in water content inside the leaves making it evident that the central parts of the leaves dry out at a lower rate than their periphery. Thus, application of sub-THz imaging is essential to perform correct water content evaluation as a leaf position is changed.

For comparison, similar experiment was carried out with the leaves separated from the same clover plant. As indicated by the red curve, cutting the leaf off causes a surge in its transmission value, signifying rapid dehydration of the detached leaf within a single day.

Another point of interest in our study was to examine the leaf water dynamics during its dehydration-watering cycle. Figure 3 shows the transmission of three grass-blade samples over a 9-day test period with a single intermediate watering on day 6. In this case, the transmission esti-

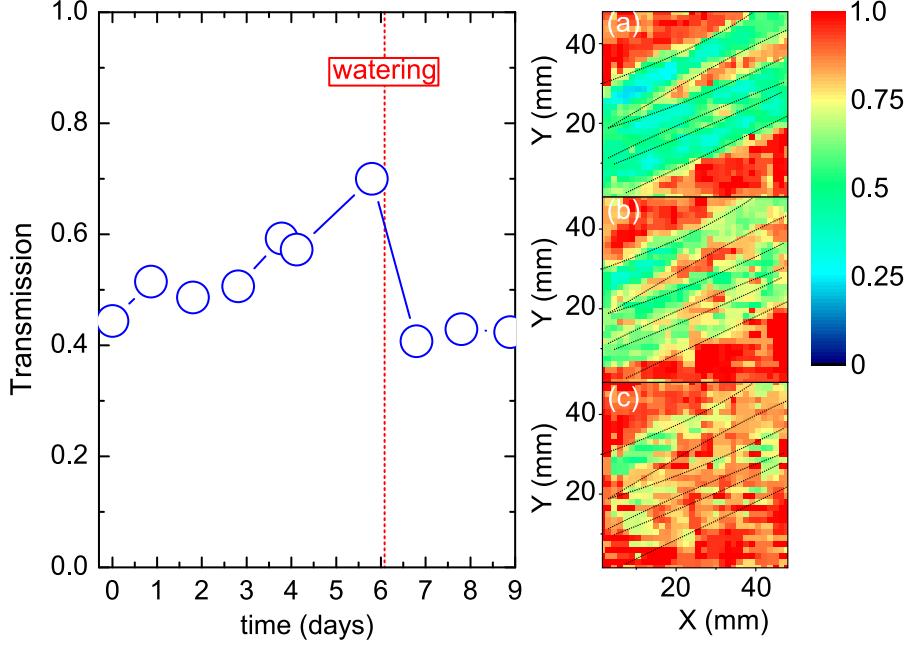


Fig 3 Changes in the transmission of a sub-THz signal through the grass blades. The blue curve with empty circles corresponds to the mean transmission values. The red dashed line marks the moment of watering the plant. Sub-THz images (a), (b), (c) illustrate various degrees of hydration of the grass blades, recorded on the first, fourth, and sixth days of the experiment, prior to the indicated watering of the plant. Image colors designate the value of the transmittance.

mate was obtained following the same averaging procedure as described above. The three images in the figure represent the transmission patterns recorded on the first, fourth, and sixth day of the experiment, during which period no water was supplied to the plant. Similar to the previous results for the clover leaves, we can see a well-established trend of an increasing transmission coefficient related to the gradual dehydration of the grass leaves.

When the grass was watered at the end of day 6, as marked by a red dashed line, the data indicates a prompt return to the initial transmission level, implying that the water content in the grass leaves is fully restored in less than a day after watering.

Since the transmission coefficient is related directly to the measure of water in plant leaves, in many agricultural applications, it is sufficient to know its value, without converting it into the actual water content. Hence, this figure can be used as a basis for estimating the other parameters

of interest, including the optimal watering schedule of the crops.

4 Conclusion

In conclusion, the TeraSense imaging system comprised of an IMPATT-diode source, a condenser lens, and an imaging camera was adapted to performing the quantitative analysis of the temporal evolution and spatial distribution of water in clover and grass leaves. The water content of leaf samples was estimated by measuring the transmission of 100 GHz radiation through the leaves. We observed the time changes in the transmission coefficient when the plants were subject to water restricted conditions. We show that watering the plants after prolonged dehydration results in prompt restoration of the transmission parameter to its initial value. The presented experimental findings demonstrate that TeraSense imaging instrumentation is fully capable of monitoring the hydration state of plants. Further development in this field of research may involve raising the radiation frequency to a higher band of 300 GHz to enhance spatial resolution. [In this case the size of the pixel would be decreased correspondingly to avoid the loss of the spatial resolution.](#) Moreover, imaging in reflection mode may enable real-time, continuous remote monitoring and control of the plants' hydration status.

Disclosures

The authors have no potential conflicts of interest to disclose.

Acknowledgments

The work was supported by the Russian Science Foundation Grant No. 19-72-30003

References

- 1 T. Crowe, T. Globus, D. Woolard, *et al.*, “Terahertz sources and detectors and their application to biological sensing,” *Philos Trans A Math Phys Eng Sci.* **362**, 365–377 (2004).
- 2 T. Löffler, T. Bauer, K. Siebert, *et al.*, “Terahertz dark-field imaging of biomedical tissue,” *Optics Express* **9**(12), 616 – 621 (2001).
- 3 P. Knobloch, C. Schildknecht, T. Kleine-Ostmann, *et al.*, “Medical thz imaging: an investigation of histo-pathological samples,” *Phys. Med. Biol.* **47**(21), 3875 – 3884 (2002).
- 4 H. Ge, Y. Jiang, Z. Xu, *et al.*, “Identification of wheat quality using thz spectrum,” *Optics Express* **22**, 12533–12544 (2014).
- 5 W. Xu, L. Xie, Z. Ye, *et al.*, “Discrimination of transgenic rice containing the cry1ab protein using terahertz spectroscopy and chemometrics,” *Scientific Reports* **5**, 11115 (2015).
- 6 B. B. Hu and M. C. Nuss, “Imaging with terahertz waves,” *Optics Letters* **20**(16), 1716–1718 (1995).
- 7 P. E. Verslues, M. Agarwal, S. Katiyar-Agarwal, *et al.*, “Methods and concepts in quantifying resistance to drought, salt and freezing, abiotic stresses that affect plant water status,” *Plant Journal* **45**, 523–539 (2006).
- 8 J. Xu, K. W. Plaxco, and S. J. Allen, “Absorption spectra of liquid water and aqueous buffers between 0.3 and 3.72 thz,” *J. Chem. Phys.* **124**, 036101 (2006).
- 9 H. J. Liebe, G. A. Hufford, and T. Manabe, “A model for the complex permittivity of water at frequencies below 1 thz,” *International Journal of Infrared and Millimeter Waves* **12**, 659–675 (1991).

- 10 B. B. Hu and M. C. Nuss, “Imaging with terahertz waves,” *Optics Letters* **20**, 1716–1718 (1995).
- 11 D. Mittleman, R. Jacobsen, and M. Nuss, “T-ray imaging,” *IEEE Journal of Selected Topics in Quantum Electronics* **2**, 679–692 (1996).
- 12 N. Born, D. Behringer, S. Liepelt, *et al.*, “Monitoring plant drought stress response using terahertz time-domain spectroscopy,” *Plant Physiology* **164**, 1571–1577 (2014).
- 13 E. Castro-Camus, M. Palomar, and A. A. Covarrubias, “Leaf water dynamics of arabidopsis thaliana monitored in-vivo using terahertz time-domain spectroscopy,” *Scientific Reports* **3**, 2910 (2013).
- 14 R. Gente, N. Born, N. Vo β , *et al.*, “Determination of leaf water content from terahertz time-domain spectroscopic data,” *Journal of Infrared, Millimeter, and Terahertz Waves* **34**, 316–323 (2013).
- 15 G. G. Hernandez-Cardoso, S. C. Rojas-Landeros, M. Alfaro-Gomez, *et al.*, “Terahertz imaging for early screening of diabetic foot syndrome: A proof of concept,” *Scientific Reports* **7**, 42124 (2017).
- 16 S. Wietzke, C. Jansen, C. Jördens, *et al.*, “Industrial applications of thz systems,” *Proceedings of SPIE - The International Society for Optical Engineering* **7385**, 738506 (2009).
- 17 M. Schwerdtfeger, E. Castro-Camus, K. Krügener, *et al.*, “Beating the wavelength limit: three-dimensional imaging of buried subwavelength fractures in sculpture and construction materials by terahertz time-domain reflection spectroscopy,” *Appl. Optics* **52**, 375–380 (2013).

- 18 H. Zhong, J. Xu, X. Xie, *et al.*, “Nondestructive defect identification with terahertz time-of-flight tomography,” *IEEE Sensors Journal* **5**, 203 – 208 (2005).
- 19 A. I. Hernandez-Serrano, S. C. Corzo-Garcia, E. Garcia-Sanchez, *et al.*, “Quality control of leather by terahertz time-domain spectroscopy,” *Appl. Optics* **53**, 7872–7876 (2014).
- 20 D. Banerjee, W. von Spiegel, M. D. Thomson, *et al.*, “Diagnosing water content in paper by terahertz radiation,” *Optics Express* **16**, 9060–9066 (2008).
- 21 K. Kawase, Y. Ogawa, Y. Watanabe, *et al.*, “Non-destructive terahertz imaging of illicit drugs using spectral fingerprints,” *Opt. Express* **11**, 2549–2554 (2003).
- 22 Y. C. Shen, T. Lo, P. F. Taday, *et al.*, “Detection and identification of explosives using terahertz pulsed spectroscopic imaging,” *Appl. Phys. Lett.* **86**, 241116 (2005).
- 23 M. Tonouchi, “Cutting-edge terahertz technology,” *Nature Photonics* **1**, 97–105 (2007).
- 24 P. Jepsen, D. Cooke, and M. Koch, “Terahertz spectroscopy and imaging - modern techniques and applications,” *Laser & Photonics Reviews* **5**, 124–166 (2010).
- 25 S. Hadjiloucas, L. Karatzas, and J. Bowen, “Measurements of leaf water content using terahertz radiation,” *IEEE Transactions on Microwave Theory and Techniques* **47**, 142 – 149 (1999).
- 26 N. Karpowicz, H. Zhong, C. Zhang, *et al.*, “Compact continuous-wave subterahertz system for inspection applications,” *Appl. Phys. Lett.* **86**, 054105 (2005).
- 27 A. Dobroiu, M. Yamashita, Y. N. Ohshima, *et al.*, “Terahertz imaging system based on a backward-wave oscillator,” *Applied Optics* **43**, 5637–5646 (2004).
- 28 Q. Song, Y. Zhao, A. Redo-Sanchez, *et al.*, “Fast continuous terahertz wave imaging system for security,” *Optics Communications* **282**, 2019–2022 (2009).

- 29 B. Breitenstein, M. Scheller, M. K. Shakfa, *et al.*, “Introducing terahertz technology into plant biology: A novel method to monitor changes in leaf water status,” *Journal of Applied Botany and Food Quality* **84**, 158 – 161 (2011).
- 30 Y. F. Sun, J. D. Sun, Y. Zhou, *et al.*, “Room temperature gan/algan self-mixing terahertz detector enhanced by resonant antennas,” *Appl. Phys. Lett.* **98**, 252103 (2011).
- 31 Y. F. Sun, J. D. Sun, Y. Zhou, *et al.*, “High-responsivity, low-noise, roomtemperature, self-mixing terahertz detector realized using floating antennas on a ganbased field-effect transistor,” *Appl. Phys. Lett.* **100**, 013506 (2012).
- 32 H. Qin, X. Li, J. Sun, *et al.*, “Detection of incoherent terahertz light using antenna-coupled high-electron-mobility field-effect transistors,” *Appl. Phys. Lett.* **110**, 171109 (2017).
- 33 G. Tsydynzhapov, V. Muravev, A. Fortunatov, *et al.*, “Commercial sub-thz video camera,” in *20th International Display Workshops 2013, IDW 2013*, 1413–1414 (2013).
- 34 V. Muravev, G. Tsydynzhapov, A. Fortunatov, *et al.*, “High-speed thz semiconductor imaging camera,” in *2013 38th International Conference on Infrared, Millimeter, and Terahertz Waves*, 6665502 (2013). [doi:10.1109/IRMMW-THz.2013.6665502].
- 35 V. M. Muravev, G. E. Tsydynzhapov, A. A. Dremin, *et al.*, “New terahertz imaging system for industrial applications,” in *2016 41st International Conference on Infrared, Millimeter, and Terahertz waves*, 7758612 (2016). [doi:10.1109/IRMMW-THz.2016.7758612].
- 36 G. E. Tsydynzhapov, P. A. Gusikhin, V. M. Muravev, *et al.*, “New terahertz security body scanner,” in *2018 43rd International Conference on Infrared, Millimeter, and Terahertz Waves*, (2018). [doi:10.1109/IRMMW-THz.2018.8510513].
- 37 M. Klein and A. J. Gasiewski, “The sensitivity of millimeter and sub-millimeter frequencies

to atmospheric temperature and water vapor variations,” in *IGARSS’98. Sensing and Managing the Environment. 1998 IEEE International Geoscience and Remote Sensing. Symposium Proceedings.*, **2**, 568–571, IEEE (1998).

- 38 V. M. Muravev and I. V. Kukushkin, “Plasmonic detector/spectrometer of subterahertz radiation based on two-dimensional electron system with embedded defect,” *Appl. Phys. Lett.* **100**, 082102 (2012).
- 39 V. M. Muravev, V. V. Solov’ev, A. A. Fortunatov, *et al.*, “On the response time of plasmonic terahertz detectors,” *Journal of Experimental and Theoretical Physics Letters* **103**, 792–794 (2016).

I.V. Kukushkin is a chief scientific researcher at the Institute of Solid State Physics RAS. He received his Ph.D. in 1983. In 1987 I.V.Kukushkin was awarded the Soviet National Prize, being recognized as the best young scientist. In 1997 he was elected a corresponding member of the Russian Academy of Sciences in General Physics and Astronomy Division. In 1999 he became a professor of Moscow State University, where he supervised over 10 Ph.D. dissertations and over 15 diploma theses. In 2001 V.Kukushkin received the International Max Planck and Alexander-von-Humboldt Research Award for “his pioneering achievements in solid-state physics and fundamental contribution to investigation of the fractional quantum Hall effect.” V.Kukushkin was the second Russian scientist to receive the first prize of the German scientific society since the institution of this award.

Biographies and photographs of the other authors are not available.